



Remote Air Intake  
Installation Instructions  
2033 & 2057

1. Mount the Remote Air Intake Manifold to the wall using the 3 1/2" mounting screws provided. See Fig 1
2. Each of the clear plastic intake tubes are then inserted into the Intake Filters of each Compressor Head.
3. Licensed plumber to route piping from equipment room to the outside of building per all applicable codes.
4. Connect the Remote Air Intake Filter Manifold to the incoming piping system. Piping may be flexible or rigid, per codes and preference.

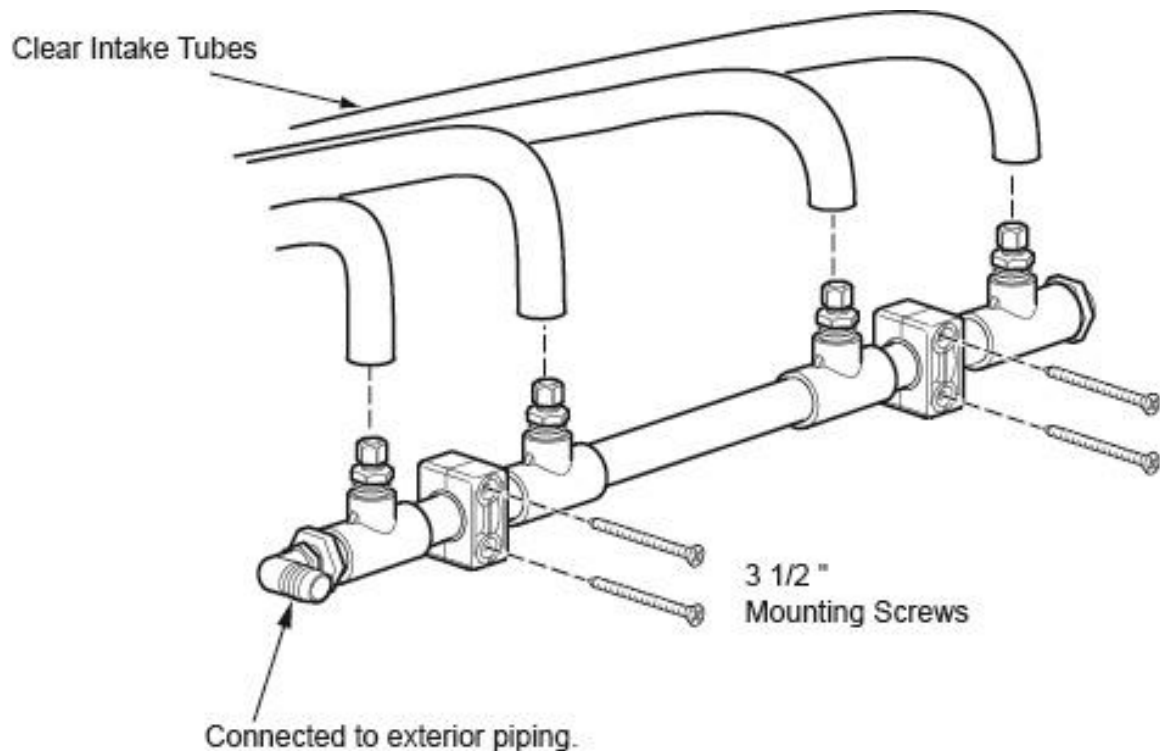


Figure 1